


RehaCom

computer-assisted cognitive rehabilitation - brain performance training



Visuo-constructive abilities

RehaCom[®]

computer-assisted cognitive rehabilitation

by Hasomed GmbH

This manual contains information about using the RehaCom therapy system.

Our therapy system RehaCom delivers tested methodologies and procedures to train brain performance .
RehaCom helps patients after stroke or brain trauma with the improvement on such important abilities like memory, attention, concentration, planning, etc.

Since 1986 we develop the therapy system progressive.
It is our aim to give you a tool which supports your work by technical competence and simple handling, to support you at clinic and practice.

HASOMED GmbH
Paul-Ecke-Str. 1
D-39114 Magdeburg
Germany

Tel. +49-391-6230112

Table of contents


Part I Training description	1
1 Training task	1
2 Performance feedback	3
3 Level of difficulty	3
4 Training parameters	4
5 Data analysis	7
Part II Theoretical concept	8
1 Foundations	8
2 Training aim	11
3 Target groups	12
4 Bibliography	14
Index	16

1 Training description

1.1 Training task

The procedure **Visuo-constructive abilities** trains the visual reconstruction of pictures of three dimensional concrete objects. Puzzles (jig-saw) are used. Each training task consists of an acquisition phase and a reproduction phase.

In the **acquisition phase** a picture can be seen on the monitor (picture 1) in which the contents have to be memorized. When the patient presses the OK-key the acquisition time ends.

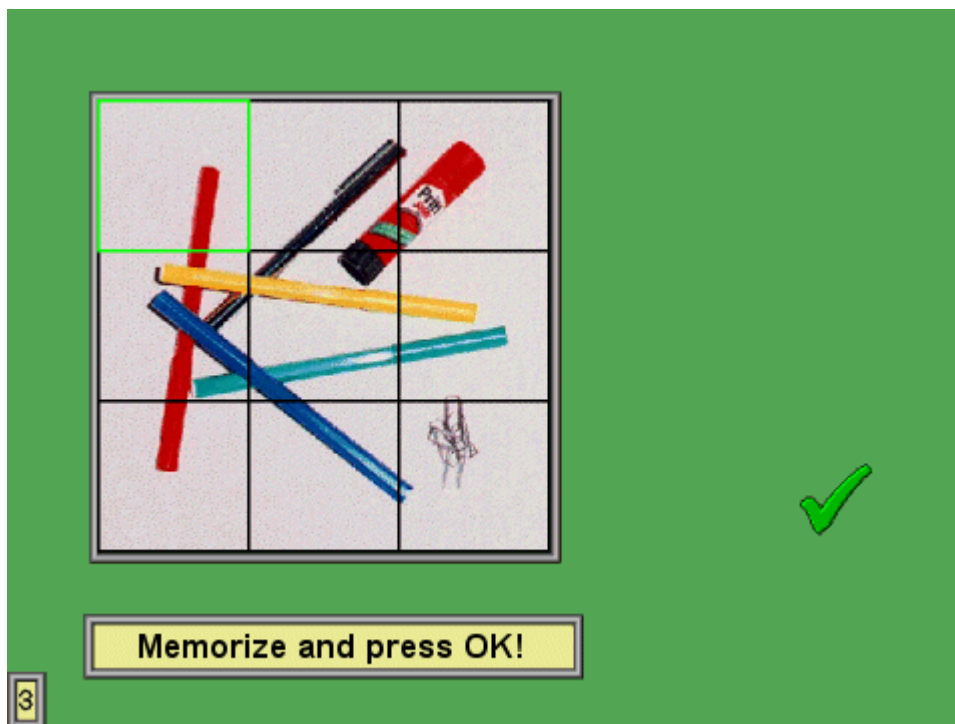


Picture 1. Acquisition phase at level 3 (Operation with the mouse).

The reproduction phase begins (Picture 2). The picture is fragmented into parts (Puzzle) and then set in a 'film' on the right hand side. A grid into which the parts have to be placed, from the 'film', is on the left hand side of the page. The **parts of the puzzle** have to be selected from the **'film' (film frame)** on the right and then placed correctly in the **grid** on the left. The reproduction phase begins - (Picture 2).

The procedure can be operated with the keyboard and/or the joystick on the RehaCom panel, with the mouse or the touch screen.

A green frame is moved by using the cursor keys on the RehaCom panel. When moving a part of the puzzle from the film frame to the grid, a green frame in the

grid must appear before the patient can press the OK-key to confirm. In this way each part of the puzzle is moved over piece by piece. If a green picture frame is moved from the left over to the right it jumps from the grid over to the film frame. A picture can now be selected from the film frame by using the keys 'arrow up' and 'arrow down'. A picture can then be selected from the film frame and after this the task is to find the right place for it in the grid on the left.

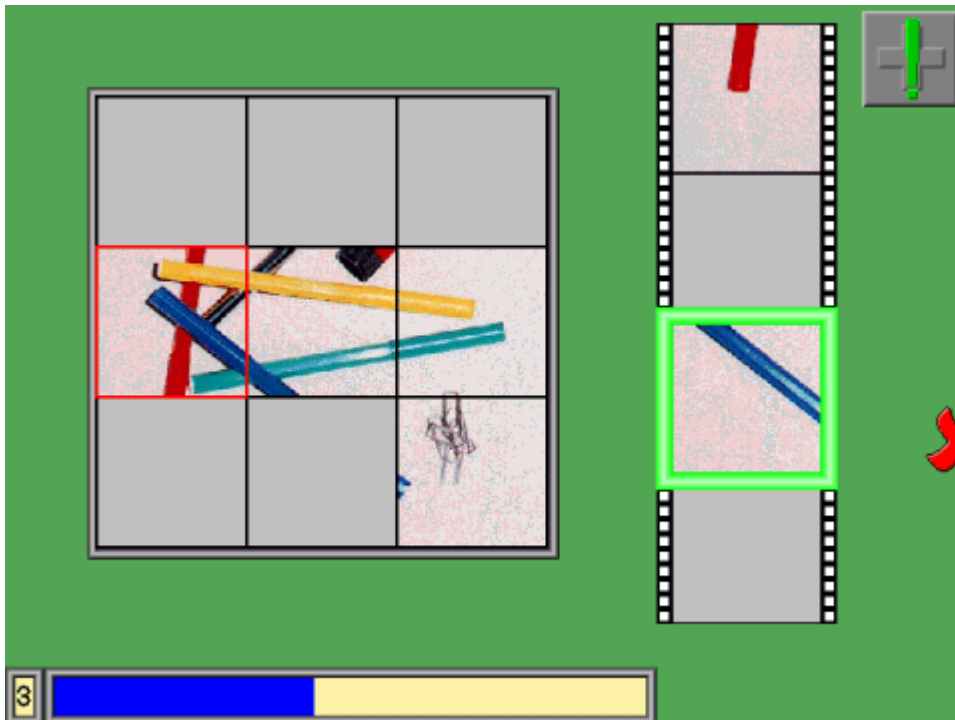

Picture 2. Reproduction phase at level 3. 4 pictures have already been sorted.
(Operation with the mouse)

The training is a lot easier with the mouse. A cursor in the form of a green arrow is used to select the correct position in the grid. By pressing the mouse button or the OK-key a picture is moved from the film frame to the selected grid position (one hand can operate the mouse; the other can press the Ok-key on the RehaCom panel). If the patient wants to move the pictures in the film frame he simply moves the cursor to the top of the film frame or the bottom of the film frame. The mouse cursor appears as a green arrow. He then presses the OK-key or the mouse button to move the pictures in the required direction. The **joystick** can be used in the same way.

Operation with the **touch screen** is easier again if there is one available. To place a picture in the grid the patient must first select the desired position in the grid and then drag the picture from the film frame on the right to the grid on the left. The pictures in the film frame can be moved when the patient touches the top or the bottom of the film frame. Alternatively, on the screen the switch with the

arrows symbols can be pressed.

At higher [levels of difficulty](#) the pictures in the film frame are turned to 90°, 180° or 270° before one has to order them to the correct position in the grid ([mental rotation](#)). A picture can only be turned when it is in the film frame. The picture can be turned with the **cursor keys** - when the picture is surrounded with a green frame it can be turned and the patient selects the correct angle by pressing the OK-key. With the **mouse** the patient simply clicks on the required picture (the cursor then changes to a rotation arrow). With the **touch screen** the picture can be rotated in the film frame or the patient can use the rotation symbols to the right of the film.

This description sounds rather complicated, but the patients learn how to operate the procedure quite quickly. At first the mouse or the touch screen method is recommended. In the instruction phase the patient has the opportunity to 'learn by doing'.

When all the pictures have been correctly sorted the patient can marvel at his work -the grid disappears. The training can be continued by pressing the OK-key. At completion of the puzzle the task is evaluated and the patient is advise as to whether a change of level should take place. The criteria for a change of level is calculated by observing the number of correct decisions in relation to the number of attempts made. A percentage is then calculated and compared to the set values for 'continue to the next level' or 'repeat the previous level' (see [Training parameters](#)).

1.2 Performance feedback

Below the screen a blue column is to be found (see picture 2). With every correct decision the column grows from left to right. The column can be switched off in the [parameter menu](#). Alongside the column the level of difficulty is shown.

If the acoustic [Feedback](#) is switched on then with each incorrect signal a error signal is heard. The acoustic feedback should switched off if there are more than one patients in the room. This prevents interference.

1.3 Level of difficulty

In order to have a very diversified training there are more than 100 pictures and photographs available. For children appropriate pictures can be used. The attractive surface supports the motivation of the patient. An adaptive set up of the procedure is guaranteed. In default setting training, the number of the puzzle parts into which the initial image is placed as well as the already mentioned [rotation](#) of the parts affects the modification of difficulty.

Further possibilities to match the procedure to the patient's performance are described in the [Training parameters](#).

Table 1 shows the levels of difficulty.

Table 1
Structure of the level of difficulty.

Level	Number of parts	Rotation
1	4	no
2	6	no
3	9	no
4	12	no
5	16	no
6	20	no
7	25	no
8	30	no
9	36	no
10	4	yes
11	6	yes
12	9	yes
13	12	yes
14	16	yes
15	20	yes
16	25	yes
17	30	yes
18	36	yes

When the patient changes from level 9 to 10 the patient gets additional tasks. The parts of the picture are turned and have to be corrected. For the most patients, the jump from 36 to 4 puzzle parts is regarded as an easier task. This is intention of the procedure developers. It should be certain that the patient only learns the extended operation - rotation of the parts -. With increasing number of the puzzle parts in the following tasks, the difficulty once again increases in a very fast way. One also no longer switches automatically back to level 9 if a patient reached level 10 with an inadequate performance.

1.4 Training parameters

In the **RehaCom basic foundations**, some general information (references) is given on the Training Parameters and their properties. This information (references) should be taken into further consideration. Picture 3 shows the


parameter-menu.

Current level of difficulty:

The level of difficulty can be set up from levels 1 to 18.

Duration of training/Consultation in mins:

A training period of 25-30 Minutes is recommended. The duration time is checked only after a task has been completed. Before the next task begins the procedure checks to see if there is enough time left over.

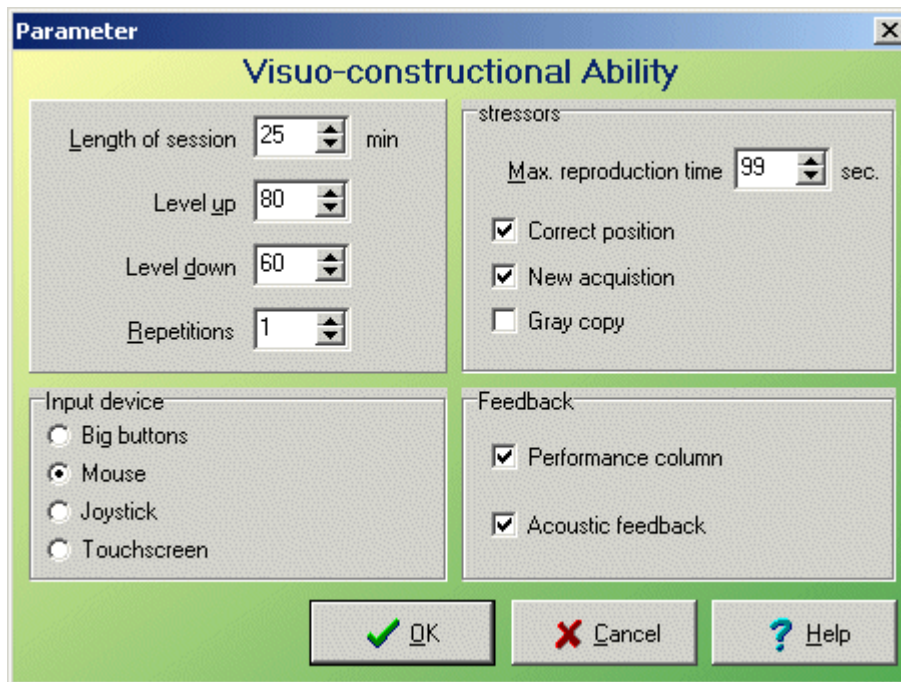

Picture 3. Parameter-Menu.

Continue to the next level, Repeat the previous level:

See [Training tasks](#).

Repetition:

The level changes if the number of established tasks with "repetitions" is successfully solved and vice versa. The level is only changed if a consolidation of performance - positive or negative - occurs. If the parameter is set to 0 the after each task is solved - the level then increases and vice versa. If a puzzle is solved without any errors, the next level is set up - there is no repetition. This acts as an additional aspect of performance assessment.

Maximum Reproduction time:

If the value for the "maximum reproduction time" is not equal to 99, an additional time stress factor is set. A clock appears which displays the remaining

time. The maximum reproduction time is calculated from the max. time multiplied by the number of pictures. If a patient does not solve a task within the maximum time then the training is broken off and the patients performance up to this point is analysed in order to give a result and an easier task is then set up.

Correct placement:

If this parameter is activated, it is then no longer possible to put a part of the puzzle in an incorrect position. After notification of error the incorrectly placed picture wanders back over to the film frame. The training becomes more difficult when this parameter is deactivated. Pictures can then be placed in the wrong position. They then have to be removed from the grid and placed back into the film frame again. In addition the green frame can be placed in the wrong position in the grid using the cursor keys and then the OK-key pressed. However, with the mouse one clicks on the picture and when the picture is placed in the grid in the wrong position the green arrow changes to a red one pointing out of the grid. With the touch screen the puzzle can be ordered by using your finger.

Renewed acquisition:

The training becomes easier when the patient operates the procedure with the renewed acquisition option. The memory aspect of the training is then lost. By pressing the "+" key on the RehaCom panel the original picture appears. When using the mouse or the touch screen there is a switch on the screen whereby this option can be used (see [Picture 2](#)). After the patient has memorized the picture again, the training can be continued by pressing the "+" key or the OK-key.

Grey-Picture:

An additional component of memory can be controlled by using the so-called "Grey-picture". If this option is activated the original picture is continuously shown as a grey-picture in the grid. The training then becomes considerably easier and becomes more dependent on comparison between the pictures in the film frame and the grid.

Input mode:

See [Schwierigkeitsstruktur](#).

Acoustic Feedback:

See [Feedback](#).

Performance Bar:

See [Feedback](#).

With each new set up of the training the following defaults are automatically installed (middle standard level):

Level of difficulty	1
Duration of training/Consultation	25 Minutes
Continue to the next level	80 %
Repeat the previous level	60 %
Input mode	Mouse
Performance bar	on
Acoustic feedback	on
Grey picture	off
renewed acquisition	on
correct placement	on
max. Reproduction time	99 s (no clock appears)
Repetition	1

1.5 Data analysis

The diverse possibilities of data analysis for the determination of the further training strategy are described in the

RehaCom basic foundations

In the pictures as well as the tables, alongside the setting for the [trainings parameter](#), the following information is available:

Level	current level of difficulty
Training time (effective)	effective Training time
Pauses	Number of pause by the patient
Number of Elements	Number of picture parts
Acquisition time.	Acquisition time in seconds (incl. renewed Acquisitions)
Reproduction time.	Reproduction time in seconds
Number. renewed Acquisition.	Number of renewed Acquisitions
position error	Number of position errors (picture was moved to the wrong place)
rotation error	Number of rotation errors (picture in right position but, was incorrectly rotated),
Number of correct selections/ Number of selections	Number of correct selections (Number of correct decisions, a picture move from film to the grid) / Number of selections (Film to Grid) = Total of correct and incorrect decisions

Number of correct parts

Number of correct parts in the puzzle (at the break of point after maximum reproduction time)

In this way it is possible to give the patient advise on their short-comings.

2 Theoretical oncept

2.1 Foundations

One defines **visual spatial performance** as perception abilities which require a visual comparison of spatial stimulus without manual effort from the patient. In contrast to this, **spatial-constructive performance** demands this exact manual-constructive component to be under visual control (cf. [Kerkhoff, Münßinger & Marquardt, 1993](#)).

According to [Kolb & Whishaw](#) deficits in the latter field for the group **visuo motor problems** those also may also include disturbances to the visual scanning and graphomotoric disturbances.

The abilities which one recognizes as being part of **visuo constructive performance** are, for example, the putting together of elements (Dice, puzzles) or the drawing of two dimensional or three dimensional figures or the spontaneous drawing of a single figure. **Spatial-constructive problems** or **constructive apraxia** refer to the decreased ability or inability in patients, with brain damaged, to draw such shapes and figures correctly and/or to join elements of a figure together to form a total figure.

According to [Goldenberg](#) (1993), in contrast to the Apraxia, this is a partial symptom of a more general impairment of spatial perception or it can also be seen as an impairment to problem solving.

The Apraxia, which according to Liepmann (1905, 1908; cf. [Goldenberg](#), 1993) can be distinguished as follows: ideomotoric (incorrect imitation of gestures) and ideatoric (incorrect results to actions and loss of knowledge about the correct use of objects). Liepmann goes on to say that these types of apraxia are related to the planning or carrying out motor actions and that in the case of unilateral lesions always also affect, in relation to the lesion, the opposite side of the body. As the medical literature is full of many different variations in the definition of apractic disturbances and that these are often seen in conjunction with other neuropsychological deficits; it may be helpful here to give an exact classification of apraxia, with the aid of clinical differentiation:

- . in relation to the affected part of the body,
- . the particular disturbance in movement

- . the error

Errors - which patients who suffer from brain damage make while copying geometrical figures, often exist in omissions or errors in positioning of individual components as well as the distorted fabrication of the presentation. In the Mosaic Test (see below) inversion or incorrect rotation often occurs. In serious cases the basic quadratic form can completely disappear. There is a similar reaction to 3 dimensional pictures (incorrect spatial rotation). The folding or cutting out of figures from paper is complicated or impossible. Length and angular distortions may also occur, size modifications or an erroneous order of individual elements of the total figure which is sometimes also reconstructed in a completely fragmented manner. In addition independent constructive abilities like the drawing of spatial orders of a room for example, with above mentioned deficits is just not possible.

Apractic problems are possibly the result of visual-spatial impairments because the precondition for **visuo constructive performance** is an intact visual-spatial perception, which helps us to deal with the world around us.

The visual-spatial perception is a component of elementary visual efficiency and consists of the following basic functions ([Kerkhoff, 1988](#)):

Visual spatial perceptive performance

- . Distance estimation (horizontal / vertical),
- . Estimation of distances,
- . Estimation of relative positions,
- . Estimation of angles,
- . Main visual spatial (subjective perpendicular / horizontal),
- . Subjective straight ahead direction / subjective middle.

Visual spatial operation

- . mental rotation,
- . Transformation performance (measure, angle, size transformations, tasks with varied spatial systems).

In contrast to the visual spatial perception, with visual room operations it is a question of cognitive services which require an intermediate step separated by the stimulus material.

Basic functions of the visual spatial perception are in everyday life, in particular in traffic, of great relevance. From the straight line directing while walking to fine motor adjustment while reading, (which are dependent on the elementary aspect

of visual performance), spatial disturbances can affect all practical everyday activities which require a visual spatial operation or a partial spatial-constructive performance. Patients with technical professions who suffer from these deficits will often lose their positions and therefore are clearly more affected than others.

Several investigations into the [predicators of the rehabilitation](#) (v. Cramon & Zihl, 1988; [Kerkhoff & Marquardt](#), 1995) showed a statistical connection between visual-constructive and visual-spatial problems and impaired ADL-activities (activities of daily living); where a causal relationship was discussed. This is not surprising when one only considers some examples from everyday life, where there is dependency on an intact visual-spatial perception and/or spatial-constructive subsets of the system:

- . Dressing
- . Folding of washing
- . Estimating and separating amounts
- . Decorating a table
- . Tidying
- . Grabbing objects
- . Estimating the depth of steps/stairs
- . Reading of plans or sketches
- . The filling in of forms and documents
- . Maintain lines and columns while drawing
- . Finding the way
- . Wheel chair navigation

More complex disturbances to perception are often a result of disturbances to the elementary visual efficiency, like the *depth perception*. Loss of depth of vision means that everything appears to be flat (e.g. a cube appears to be a six cornered object). The trouble with disturbances to depth of vision is that it is sometimes combined with changes in the perception of the sizes of objects (Micropsia and Macropsia), however, it can also affect the appearance of objects and faces. The latter is also to be seen in the case of cerebral amblyopia, problems with the shaping and colour perception which occurs in most cases after post-chiasmatic injuries.

A damaged visual localization of stimulus affects the appraisal of distances. The patient then over- or under-estimates distances.

Visual-spatial orientation problems express themselves in the loss of the spatial organization of a pattern of stimuli, which is often coupled with "difficulties in measuring" through impairments in the recognition or localizing of spatial

positions and regions as well as the *ability for spatial imagination*. Therefore, finding a way is also complicated in the case of the labyrinth tasks.

An innate medical history of the complaints is reasonable only with patients without visual neglect, anosognosia or anosodiaphoria. For the patient group with reduced insight Kerkhoff & Blaut have developed (1992, cf. [Kerkhoff, Münßinger & Marquardt](#), 1993) a clinical hetero-medical history curve. For the diagnosis of performance in visual-spatial perception, the following tests are suitable, for example line orientation, line halving, spatial sub tests in intelligence tests or the computer-assisted procedure is also suitable (cf. [Kerkhoff, Münßinger & Marquardt](#), 1993). The latter registers elementary performances of the visual spatial perception in contrast to all other procedures. The tests for visual object and spatial perceptions (VOSP, [Warrington & James](#), 1992) also tests the visual basic functions problems which often occur together with constructive apraxia and are possibly its cause. For the diagnosis of the spatial-constructive troubles - the free copying of geometric or other patterns, the copying of perspective drawings or the drawing test according to [Grossmann](#) (1988) are suitable. The mosaic test or the sub test 'figure placing' from the Hamburg change/switching intelligence test (HAWIE-R, [Tewes](#) 1991), the Benton-Test ([Benton](#), 1981) or the Rey-Osterrieth-Figur ([Osterrieth](#), 1944) are also suitable as diagnostic instruments. However there are in part particular aspects; partial combination of many aspects of more complex functions registered. i.e. several spatial basic functions are tested simultaneously.

2.2 Training aim

The aim of the training is to improve the patient's [visuo constructive performance](#). This computer training helps to improve functions and abilities required in everyday life; as it is highly probable that visuo constructive impairments occur as a result of deficits to the basic performance of perception.

In training puzzles are used which must be memorized and reconstructed. In this way, the visual memory is supported in addition to training visuo-constructive abilities. If required, less emphasis can be placed on the aspect of memory in that the patient can constantly refer to the [grey picture](#) or there is also the possibility to refer back to the original picture and to match this with his current version of the puzzle.

The segmentation of the matrix is simultaneously a starting point for the procurement of strategy - the division of more complex drafts into components is useful as in the case of copying or re-creating.

It is to be expected that the improvement of visual-spatial [basic functions](#) may have a positive affect on that ADL- field (Activities of Daily Living).

Impairments to the spatial perception and to the spatial operations hinder numerous practical activities (eating, dressing, body-care, writing, drawing, car driving), in particular if it depends on a precise type of visuo-motor co-ordination. Furthermore, there are significant statistical connections between mosaic test and figure batching (HAWIE) and the ADL measures (cf. [Kerkhoff, 1988](#)), so that may first be employed as predicators for independence in everyday life. On the basis of the maximum specification of therapy, one should always precede with a differentiated problem specific neuropsychological [diagnostic](#).

A good preparation for training with the procedure **Visuo-construction** is to practice with the procedure RAUM. The aim of the latter procedure is the specific training of basic visual-spatial single performances and the estimating of angles, the positioning of subjects as well as the appraisal of sizes and faces. In this case, emphasis was placed on the closeness to reality of the tasks as in, for example, the filling of vessels of different forms. Each single procedure concentrates itself on a component visual-spatial basic functions while the demand on other intellectual abilities was kept to a minimum.

In consideration of the lack of methods to diagnose and handle visual [spatial perceptions](#) and the disturbances to [spatial operations](#), the procedure also offers the possibility of a more differentiated recording of the underlying problems.

For additional training, the RehaCom-Procedures **Spatial Operation** (RAUM), **Visuo-Motor Co-ordination** (WISO) and **Two dimensional Operationen** (VOR1) can be used.

Due to the complexity of the procedure it may also be used in the areas of **Attention** and **figurative memory** in connection with the RehaCom-Training procedures (AUFM, GEAU).

2.3 Target groups

It is recommended that the procedure be used to train the [visuo-constructive abilities](#) of patients with diagnosed impairments to the performance visual spatial [perception](#) and disturbances to their spatial-constructive abilities.

It is mainly patients whose brain has been damaged after posterior and/or parieto-occipital uni- and bilateral lesions or injuries to the visual system, who are affected. In particular visual-spatial problems often occur after right-hand parietal lesions.

Visual-spatial functions can be affected by different types of brain damage of different genesis (insult, hypoxia, SHT, tumours).

The patients who will also benefit from a training of spatial functions are certainly those with visual neglect, impairments to field of vision and those with impairments to their object perception caused by deficits in [elementary visual performance](#). The latter is also the case, when we refer to cerebral amblyopia (difficulties with shape and colour perception) which mostly occurs after postchiasmatic injuries.

Furthermore, the procedure can be employed as a type of problem solving training.

For patients with to the right hemispheric injuries to the brain there is a clear indication of a covariance between impairments to the visual spatial perception and visual constructive problems (cf. [Kerkhoff](#), 1988). Also a decreased ability for [mental rotation](#), which is observed after right- and left hemispheric posterior lesions, impairs the visual constructive performance.

In addition to a half-side paralysis, visual-constructive and visual-spatial problems is the most important predictor for the rehabilitation process in patients with injuries the right hemi-sphere of the brain.

It was repeatedly found, that in particular patient groups with deficits to visual perception a less favourable rehabilitation process was observed in the left hemispheric hemiplegia (cf. [Kerkhoff](#), 1988).

Patient's who suffer from hemiplegia often experience motor problems in their dominant hand. The procedure Kons can help to improve the dexterity of the other hand.

As per the [standard parameters](#) , the training requires the visual memory to store the picture presented in the acquisition stage in memory for so long until it has to be reconstructed. Therefore, the procedure can be used with patients with problematic visual memory performance which occurs in patients with brain damages of different localization and genesis - but predominantly in patients with right hemispheric insults, tumours and traumas.

For patients with weak memory performance, a permanent a gray image of the target image can be used or depending on set up in the [training parameter](#) the initial image may also be used.

It is possible to put the procedure to use with children of 8 years and older. It is then recommended that relevant pictures and instructions be used for the children and that, at least the first training session should be gone through with the support of a therapist.

From a diagnostic point of view it is recommended to exclude those patients with serious deficits in Intelligence.

2.4 Bibliography

Benton, A.L. (1981): Der Benton Test. Handbuch. Bern: Huber.

Boettcher, S. (1991): Zusammenhänge zwischen visuell-räumlichen und visuo-konstruktiven Leistungseinbußen bei Patienten mit Hirnschädigung und psychiatrischen Patienten. Zeitschrift für Neuropsychologie, Vol. 2 (1), S. 3-13.

Canavan, A. & Sartory, G. (1990): Klinische Neuropsychologie. Stuttgart: Ferdinand Enke Verlag.

Cramon, D.Y. von & Zihl, J. (Hrsg.) (1988): Neuropsychologische Rehabilitation. Berlin: Springer-Verlag.

Cramon, D. Y. von (1991): Sehen. In: von Cramon, D. Y. von & Zihl, J (Hrsg.). Neuropsychologische Rehabilitation. Berlin: Springer-Verlag. S. 105-129.

Goldenberg, G. (1993): Praxis. In: In: Cramon, D.Y. von, Mai, N, & Ziegler, W. (Hrsg.): Neuropsychologische Diagnostik. Weinheim: Chapman & Hall.

Grossmann, M. (1988): Drawing deficits in brain-damaged patients' freehand pictures. Brain Cog., Vol. 8, S. 189-205.

Hardesty, A. & Lauber, H. (1956): Hamburg-Wechsler-Intelligenz-Test für Erwachsene (HAWIE). Bern: Huber-Verlag.

Hartje, W. & Sturm, W. (1989): Räumliche Orientierungsstörungen und konstruktive Apraxie. In: Poeck, K. (Hrsg.): Klinische Neuropsychologie. Stuttgart, New York: Thieme Verlag.

Heilman, K. M. & Valenstein, E. (Eds.): Clinical Neuropsychology. New York: Oxford University Press.

Kerkhoff, G. (1988): Visuelle Raumwahrnehmung und Raumoperationen. In: Cramon, D. Y. von & Zihl, J (Hrsg.): Neuropsychologische Rehabilitation. Berlin: Springer-Verlag. S. 197-214.

Kerkhoff, G. (1989): Störungen der visuellen Raumwahrnehmung bei Patienten mit Hirnschädigung. Frankfurt am Main: Haag und Herchen Verlag.

Kerkhoff, G. & Marquardt, C. (1995): Quantitative Erfassung visuell-räumlicher Wahrnehmungsleistungen in der Neurorehabilitation. Neurol. Rehabil., Vol. 2.,

S. 101-106.

Kerkhoff, G., Münßinger, U. & Marquardt, C. (1993): Sehen. In: Cramon, D.Y. von, Mai, N. & Ziegler, W. (Hrsg.): Neuropsychologische Diagnostik. Weinheim: Chapman & Hall.

Kolb & Whishaw (1990): Fundamentals Of Human Neuropsychology. New York: W. H. Freeman and Company.

Marquardt, C. & Kerkhoff, G. (1994). VS - Computerunterstützte Erfassung visuell-räumlicher Wahrnehmungsleistungen. Version 2.0. Bedienungshandbuch. München.

Münßinger, U. & Kerkhoff, G. (1993): Therapie räumlich-konstruktiver und räumlich-visueller Störungen bei hirngeschädigten Patienten. Praxis Ergotherapie, Vol. 6. S. 215-221.

Osterrieth, P.A. (1944): Le test de copie d'une figure complexe. Arch. Psychol., Vol. 30, S 206-353.

Poeck, K. (Hrsg.) (1989): Klinische Neuropsychologie. Stuttgart, New York: Thieme Verlag.

Strauss, H. (1924): Über konstruktive Apraxie. Monatsschr. Psychiatr. Neurol., Vol. 50, S. 65-124.

Warrington, E.K. & James, M. (1992): VOSP - Testbatterie für visuelle Objekt- und Raumwahrnehmung. Thames Valley Test Company (Deutsche Übersetzung).

Index

- A -

Acoustic feedback 3
Acquisition phase 1
Acquisition time 7
Activities of Daily Living (ADL) 8, 11
Acoustic feedback 4
Adaptivity 3
Aetiology 12
Aim of the training 11
Apraxia 8

- B -

Basic performance 8
Basic theory 8
Bibliography 14
Brain damage 12

- C -

Closeness to reality 11
Constructive Apraxia 8
Continue to the next level 4
Continuous data analysis 7
Continuous consultation 7
Correct placement 4
Cortex areal 12
Current level of difficulty 4

- D -

Data analysis 7
Defination of a term 8
Description of the training 1
Development of strategy 11
Disturbances to memory 11
Duration of training/Cons. in mins 4

- E -

Extrinsical medical history 8

- F -

Field of vision 12
Foundations 8

- G -

Grey picture 4

- I -

Impairments to perception 8
Independance 11
Individual medical history 8
Input method 1
Input mode 4

- L -

Level of difficulty 3, 7

- M -

Maximum Reproduction time 4
Memory 4
Mental rotation 1, 8, 12

- N -

Neglect 12
Neuropsychological diagnostic 8, 11, 12
Number of correct decisions 7
Number of incorrect decisions 7
Number of pauses 7
Number of puzzles 7

- O -

Operation 1

- P -

Performance bar 4
 Performance column 3
 Performance feedback 3
 Position error 7
 Practical uses 11
 Predicator 12
 Problem solving training 12
 Process of rehabilitation 12
 Puzzle 1, 3

Visual spatial operation 8, 11
 Visual spatial perception 11, 12
 Visual spatial performance perception 8
 Visuo-constructive abilities 1
 Visuo-constructive performance 11
 Visuo-motor co-ordination 11
 Visuo-motoric disturbances 8

- R -

Reconstruction 1
 RehaCom-Procedure 11
 Renewed Acquisition 4, 7
 Repeat previous level 4
 Repetition 4
 Reproduction phase 1
 Reproduktion time 7
 Rotation 3, 7
 Rotation error 7

- S -

Spatial-constructive impairments 12
 Spatial-constructive performance 8
 Specifics of the Trainings 12
 Structure of the level of difficulty 3

- T -

Target groups 12
 Training aim 11
 Training parameter 4
 Training parameters 4
 Training task 1
 Training tasks 1
 Training time 7

- V -

Visual deficits 12
 Visual memory performance 12